

(19)



Europäisches Patentamt  
European Patent Office  
Office européen des brevets



(11)

**EP 1 369 099 A2**

(12)

**EUROPEAN PATENT APPLICATION**

(43) Date of publication:  
10.12.2003 Bulletin 2003/50

(51) Int Cl.<sup>7</sup>: **A61F 2/06**, C25D 17/06

(21) Application number: **03253608.8**

(22) Date of filing: **06.06.2003**

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR  
HU IE IT LI LU MC NL PT RO SE SI SK TR**  
Designated Extension States:  
**AL LT LV MK**

(72) Inventor: **Swain, Brian**  
**Tamworth, Staffordshire B77 5AS (GB)**


(74) Representative: **Lawrence, John**  
**Barker Brettell**  
**138 Hagley Road**  
**Edgbaston**  
**Birmingham B16 9PW (GB)**

(30) Priority: **06.06.2002 GB 0212909**

(71) Applicant: **Anopol Limited**  
**Birmingham B5 5QJ (GB)**

**(54) Improvements in stent manufacture**

(57) Stents (2) to be processed in one or more liquid baths are placed on a jig (1) comprising a plurality of wire electrodes (4) in such manner that each electrode (4) passes through and projects beyond the full length of a stent (2) placed thereon. The stents (2) carried by the jig (1) are immersed in a liquid bath which contains an electrolyte and the stents (2) are urged into contact with their associated electrodes (4) while current is applied to those electrodes. The positions of contact between the stents (2) and their respective electrodes (4) are altered during processing without removing the stents from the jig (1). The method is applicable for electro polishing and electro-plating. The stents (2) may remain on the same jig (1) throughout processing. Also disclosed is a jig (1) suitable for performing the method and comprising an electrode support member (3) holding a plurality of generally parallel wire electrodes (4) each of which passes through a hole (5) in a stent support bar (6), means for moving the stent support bar (6) towards or away from the electrode support member (3) in a direction along the electrodes (4). The wire electrodes (4) each have a diameter less than the internal diameter of the stents (2) to be processed, and they extend beyond the stent support bar (6) by a distance which is greater than the length of the stents (2). A plurality of contact positioning members (7) are movable in relation to the electrodes (4) for urging contact between each such electrode (4) and a stent (2) carried thereby.

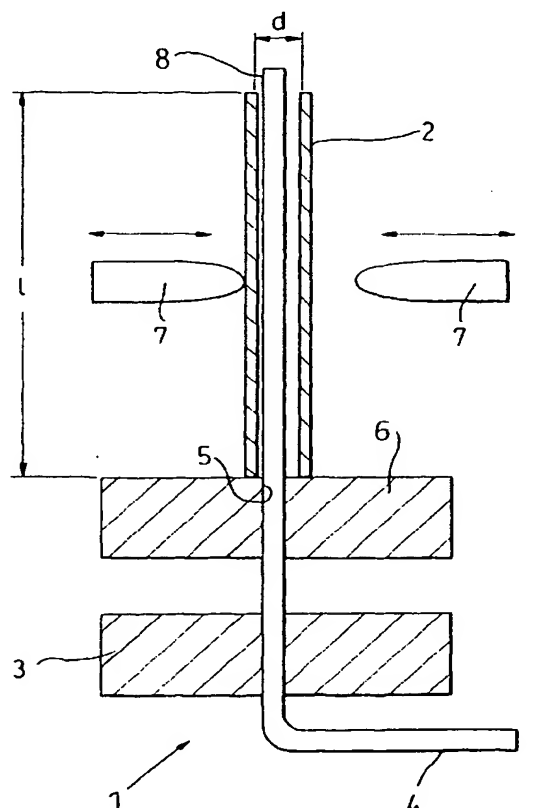**BEST AVAILABLE COPY****Fig. 2**

## Description

[0001] This invention relates to the manufacture of stents. The invention provides a new method of processing stents in at least one liquid bath, to a jig for supporting stents during such processing, processing equipment incorporating the new jig, and to stents so manufactured.

[0002] Stents used for implantation into veins or arteries are typically lattice-walled tubes which are extremely fragile. The basic manufacturing process typically leaves burrs on the walls of the stent which must be removed prior to use. The removal of these burrs is typically performed electrolytically (e.g. by electropolishing).

[0003] Hitherto, in order to remove such burrs, an electrode held on a jig has been inserted into one end of the stent and the stent has been immersed in an acid bath for electrode erosion of the burrs. Because of the fragility of the stent it is necessary that the electrode used should make contact with the interior of the stent, and electrodes used have hitherto taken the form of a bent wire or a pair of expanding tweezers which are inserted into the stent end. In an attempt to obtain a uniform treatment of the stent it has been necessary to remove it from the electrode during the course of any active treatment and to replace the stent so that the electrode is located at its other end. This is time consuming. Because stents are so fragile, they are apt to become damaged during this reversal process. Considerable skill is required in order to remove and replace the stents in this way. Furthermore, of course the fact that the electrodes are located at each of the two ends for approximately half of the processing operation will entail that the ends of the stent are processed in a different manner from the remainder of its length.

[0004] Analogous problems arise if it is desired to electro-plate a stent.

[0005] It is an object of the present invention to provide a new method for processing stents.

[0006] According to the present invention there is provided a method of processing stents in at least one liquid bath, wherein stents to be processed are placed on a jig comprising a plurality of wire electrodes, preferably in such manner that each electrode passes through and projects beyond the full length of a stent placed thereon, wherein stents carried by the jig are immersed in a liquid bath which contains an electrolyte and the stents are urged into contact with their associated electrodes while current is applied to those electrodes, and wherein positions of contact between the stents and their respective electrodes are altered during electrolysis without removing the stents from the jig.

[0007] The invention also includes a jig for supporting stents of pre-determined length ( $l$ ) and internal diameter ( $d$ ) during processing in a liquid medium which jig comprises an electrode support member holding a plurality of generally parallel wire electrodes each of which pass-

es through a hole in a stent support bar, means for moving the stent support bar towards or away from the electrode support member in a direction along the electrodes, the wire electrodes having a diameter which is less than the predetermined stent internal diameter ( $d$ ) and a length such that they can extend beyond the stent support bar by a distance which is greater than the predetermined stent length ( $l$ ), and further comprising a plurality of contact positioning members selectively movable in relation to the electrodes for urging contact between each such electrode and a stent carried thereby.

[0008] Because the electrode runs the full length of the stent during processing any contact marking between the stents and the electrode will be more evenly distributed along the stent, and this is the more so because the positions of contact between the stents and their respective electrodes are altered during the processing. The stents remain supported by the electrodes throughout the electrolytic processing step. Accordingly no time is wasted in removing the stents from the bath and reversing them on the electrodes. This also avoids any risk of damage during such a reversing step. Risks of a local burning of the stent are substantially reduced by ensuring that the end of the electrode projects through and beyond the full length of the stent. The stents will be substantially free from signs of non-uniform electrolytic contact at their ends.

[0009] Preferably, processing of the stents is performed in a succession of liquid baths while the stents are carried by the same jig, and in the most preferred embodiments of the invention, processing of the stents is performed in a succession of liquid baths, and all liquid-bath processing steps are performed while the stents are carried by the same jig. The adoption of one or both of these preferred features further reduces time which might be lost by reversing the stents on a jig and a consequent risk of damage to the stents. The requirement for skilled workers with a high degree of manual dexterity is also reduced. The processing steps may comprise pre-processing the stents prior to electropolishing or electroplating. For example, the stents may be cleaned as a pre-processing step (e.g. in an ultrasonic cleaning bath). The stents may be cleaned after electropolishing or electroplating.

[0010] While the present invention was made with particular reference to problems encountered in electropolishing stents, it is equally applicable for use during an electro-plating process. It is also applicable to other treatments of stents as part of the manufacturing process, such as cleaning steps, or surface treatment steps.

[0011] Preferably, the electrode support member, the stent support bar and the contact positioning members are formed of one or more non-conductive, acid-resistant material. The jig is thus suitable for use in electrolytic processes involving the use of an acidic electrolytic bath, as well as in other processes such as multi-stage rinsing processes. Individual control of the electrodes is enabled, and the contact positioning members will be

least likely to have any effect on the process conducted.

**[0012]** Particularly suitable non-conductive, acid-resistant material(s) include high density polyethylene, polytetrafluoroethylene, polyvinylchloride, polyvinylidifluoride, polypropylene.

**[0013]** The electrodes are suitably formed of platinum wire.

**[0014]** Preferably, said stent support bar is movable between first and second positions and said contact positioning members are located at a distance of between  $1/3$  and  $2/3$  from the nearer of such positions,  $1/3$  being the predetermined stent length. This insures that the stent is urged against the electrode wire at a median position along its length, and this in turn promotes a greater contact area between the stent and the electrode. This further promotes uniform treatment of the stent.

**[0015]** In some preferred embodiments of the invention, means is provided for moving said contact positioning members to-and-fro in a direction generally parallel to the stent support bar. In this way contact will take place between the stent and the wire electrode at opposed positions on the inner wall of the stent.

**[0016]** In other preferred embodiments of the invention, said contact positioning members are annular and means is provided for moving them in an orbital manner about the wire electrodes. In that way contact positions between the electrode wire and the inner wall of the stent can be moved around the whole of the inner wall of the stent. Such contact position can be changed intermittently or continuously. This further promotes uniformity of treatment of the stent along its length.

**[0017]** Uniformity of contact between the inner wall of the stent and the wire electrode is further promoted when each said electrode is constituted by a smooth round wire, as is preferred.

**[0018]** The invention further extends to a stent processing plant incorporating a plurality of stent processing baths, at least one jig as herein defined, and means for transporting a said jig and immersing it in the successive processing baths.

**[0019]** According to a further aspect of the invention, there is provided a method of processing a stent in a liquid bath comprising holding a wall of the stent between an inner member extending into the stent and engaging an inner surface of the wall of the stent and an outer member engaging an outer surface of the wall of the stent; and changing the contact positions at which the inner and outer members contact the wall of the stent so as to expose that part of the wall that was previously obscured by the members, the changing of the contact positions being performed without removing the stent from the inner member.

**[0020]** Preferably, the diameter of the inner member is substantially less than the internal diameter of the stent, and in which changing of the contact positions is effected by relative movement between the inner member and the wall of the stent so as to disengage the inner member from a first portion of the inner wall of the stent

and engage it with a different second portion of the inner wall of the stent.

**[0021]** Preferably, the relative movement occurs in a plane that is generally normal to an elongate direction of the inner member, more preferably the relative movement is generally in a straight line and further still the relative movement is substantially along a diameter of the stent.

**[0022]** Preferably, the inner member comprises an elongate wire or rod of substantially smaller cross-sectional area than the cross-sectional area of the stent, and moving the position of the inner member within the cross-sectional area of the stent between a first and second, different, position.

**[0023]** Preferably, the inner and outer members contact the stent wall at the same position of the stent wall so as to react contact force directly through a gripped portion of stent wall, without reacting contact force through other non-gripped positions of the stent wall.

**[0024]** According to a further aspect of the invention, there is provided a liquid bath treatment jig adapted to treat stents, the jig comprising: a set of a plurality of first stent-engaging formations adapted to be inserted inside respective stents; a complementary set of a plurality of second stent-engaging formations adapted to engage an outside wall of respective stents; pairs of first and second formations being adapted to hold a stent between them at a first position on the stent, when the formations are in a first position relative to each other; pairs of the first and second formations being adapted to hold a stent at a different, second, position on the stent so as to expose said first position on the stent, in use, to liquid of the bath, when the formations are in a second position relative to each other; and in which movement of the sets of first stent-engaging formations relative to the second set of stent-engaging formations is adapted to occur without removing the stents from the first formations.

**[0025]** Preferably, the first and second sets of formations are adapted to move in a straight line relative to each other between the first and second relative positions.

**[0026]** Preferably, a stent support is adapted to support the stents in place whilst relative movement between the first and second formations occurs.

**[0027]** Preferably, the stents are adapted to be moved laterally relative to the first formations which extend into them in use.

**[0028]** Preferably, a comb of second formations is carried by a carrier and is adapted to be moved relative to an array of first formations so as to move said second formations simultaneously.

**[0029]** Preferably, an array of first formations are adapted to be moved simultaneously relative to said second formations.

**[0030]** A preferred embodiment of the invention will now be described with reference to the accompanying diagrammatic drawings of which:-

**Figures 1A and 1B** show prior art ways of holding stents for electropolishing;

**Figure 2** shows a stent located on an electrode of a jig in accordance with one aspect of this invention;

**Figure 3** shows more structure of the jig of Figure 2;

**Figure 4** shows schematically a stent electrolytic treatment closed system incorporating the jig of Figure 2;

**Figures 5A and 5B** show alternative arrangements of the jig of Figure 2;

**Figures 6A and 6B** show alternative arrangements;

**Figure 7** shows another feature of the embodiment of Figure 2; and

**Figure 8** shows a modification.

**[0031]** Figures 1A and 1B show a stent, referenced 2, supported as in the prior art at one end only by a sprung clip C inserted into the end of the stent. In the case of Figure 1A the clip is a bent piece of spring wire. In the case of Figure 1B, it is a pair of tweezers that are spring-biased to open.

**[0032]** In Figure 2 is shown our new jig 1 for supporting stents 2 of a pre-determined length  $l$  and internal diameter  $d$ . The jig comprises an electrode support member 3 holding a plurality of generally parallel wire electrodes 4 (or first members) each of which passes through a hole 5 in a stent support bar 6 of plastics, non-conducting, material. The wire electrode 4 has a diameter which is less than the internal diameter  $d$  of the stent and the stent is accordingly a loose fit on the electrode wire. Contact positioning members 7 (or second members) which are movable to and fro in a direction along the stent support bar 6 are arranged to urge one side of the inner wall of the stent, or the other, against the electrode 4. The members 7 are also made of non-conducting plastics material.

**[0033]** In operation, stents 2 are slipped over wire electrodes 4 and come to rest on the stent support bar 6. The stent support bar is raised or lowered so that a median portion of the stent 2 is aligned with the contact positioning members 7. The contact positioning members 7 may then be urged to one side or other so as to pin the stent against the electrode 4, whereupon the stent support bar 6 may be lowered out of contact with the stent so that it does not interfere with any treatment of the stent. The stent is pinned strongly enough to prevent it from sliding down, but not so strongly as to damage the wall of the stent.

**[0034]** Because the wire electrode 4 is long enough that its end 8 projects beyond the end of the stent, any

irregularities or deformations of that end 8 of the wire electrode will not affect the processing carried out on the stent. In other embodiments, the wire 8 need not extend beyond the end of the stent; just into it.

**[0035]** Given a suitably precise construction and movement of the parts of the jig it is possible to insure that the stent will be in contact with the wire electrode 4 over substantially the whole length of the stent. This militates against any irregularity of treatment along the length of the stent. At a suitable stage during the processing the stent support bar 6 may be raised to contact the base of the stent 2, to support the stent, and the contact positioning members may be moved across to bring the other side of the stent into contact with the electrode. In an alternative arrangement the contact positioning members are moved across to pin a different part of the stent wall, without previously supporting the bottom of the stent. The stent may slide down the electrode 8, possibly to rest upon bar 6, whilst the pinning position is changed.

**[0036]** Movement of the various parts of the jig is suitably effected by one or more stepper motors, which may be controlled by a common microprocessor controller. A user may be able to select, or input, processing times or other control operations. A user-input interface (e.g. keyboard) may be provided.

**[0037]** In a variant embodiment, shown in Figure 6B, the contact positioning members 7 are each constituted by an annulus which is movable in an orbital manner, either stepwise or continuously, around the wire electrode 4 in order to vary the contact position between the stent 2 and the electrode 4 either stepwise or continually.

**[0038]** Adoption of the present invention in the electro polishing of stents primarily eliminates the need to turn the stent over. It may also give a reduced tendency of burning of the stent and may reduce any tendency to a differential polishing along the length of the stent. In particular, a stent manufactured using a jig in accordance with the invention can be substantially free from signs of non-uniform electrolytic contact at its ends.

**[0039]** Because stents do not require to be removed from the jig at any stage during the processing, it is relatively easy to construct a plant in which all the required processing baths are contained within a fume cupboard. This is plainly beneficial for the environment of those operating the plant. One or more of, or all of, reduced manufacturing times, labour costs, stent damage due to turning it over on its electrode, may also be achievable by embodiments of the invention.

**[0040]** Figure 2 shows the ends of the contact positioning members 7 as being rounded and smooth. This helps prevent damaging the stent.

**[0041]** Figure 3 shows a part of the jig 1. The jig may have about 20-30 tines of a comb-like structure 30, with each tine 31 comprising a strut 32 extending from a support bar 34, and having a contact positioning member 7 at the foot of the tine. A stepper motor 36 is shown to

control the lateral position of the comb 30.

**[0042]** A stepper motor 38 is shown to control the height of the support bar 6 relative to the contact positioning member 7.

**[0043]** An optional stepper motor 40 is shown to control the height of the electrode support member 3 relative to the contact positioning members 7.

**[0044]** A microprocessor 42 controls the stepper motors.

**[0045]** Figure 4 shows an enclosed cabinet 44 (schematically represented by chain dotted line 46) which has atmosphere control for the processes that occur inside it. The cabinet 44 has a stent treatment line inside it, including a jig 1 in accordance with the invention. The treatment line has a first pre-treatment liquid bath 50, a cleaning bath 52, an electropolishing bath 54, and a second cleaning bath 56.

**[0046]** The jig 1 is supported by, and driven on, rails 58 and can move from bath to bath, and the jig can be raised and lowered into each bath.

**[0047]** The contact positioning members 7 can be set to a third, neutral, position relative to the electrode 8, in which no force is applied to the side wall of the stent. Indeed, the side walls of the stent may not touch the contact positioning members: the stent is "loose" on the first member. This is shown in Figure 7. As can be seen there is space, or can be space, between the inner walls of the stent and the electrode. In this "non-biased" position liquid in a liquid bath can contact all curved surfaces of the stent. This can be useful in a cleaning, or other pre-treatment, operation where good electrical contact with the stent is not necessary. Indeed, we have a machine and process in which the same jig is used to carry the stents for pre-treatment steps as is used during electropolishing (or electroplating). This removes the need to transfer stents from one jig to another (as is done in the prior art). This may constitute a separate inventive step, and protection for that concept is sought.

**[0048]** Figure 6A shows an arrangement where it is the contact support member 7 that moves and pushes the stent into the opposite side of the electrode 8, with the electrode being stationary.

**[0049]** Figure 5A shows an arrangement where the first member 8 is an electrode and the contact support member is non-conductive. Figure 5B shows the opposite: the contact support member, or second member, is an electrode (shown by "+/-"), and the first member, inside the stent, is non-conductive. Alternatively the first member and the second member may be conductive. It is preferred to have the arrangement of Figure 5A.

**[0050]** The contact support member 7 may itself have a substantial elongate extent, and may comprise a wire or rod. The stent may be held between two wires/rods extending parallel to each other.

**[0051]** Figures 8A to 8C show an arrangement where it is the electrode, or first member 8, that moves, and the contact support member 7 that remains stationary. Of course, both the contact support member and first

member may move.

**[0052]** Stents come in different diameters and lengths. For example, 0.5mm diameter to 2mm diameter, and from 5mm to 40mm in length. The precise dimensions are not important to the point being made now. The same jig, with the same first and second members, is suitable for a wide variety of lengths and diameters of stents. This is not true of the prior art, where the strength of the spring force applied to the stent was chosen to suit a stent of a specific diameter. Reacting the pinning force directly through the wall helps in this regard.

**[0053]** Although we have shown the same first member contacting two different parts of the inner stent wall at different times, we could of course use two different first members: one for each position of contact. Protection for this is sought, and "first member" should be read so as to include different members at different times.

## Claims

1. A jig (1) for supporting one or more stents (2) of predetermined length (*l*) and internal diameter (*d*) during processing in a liquid medium which jig (1) comprises an electrode support member (3) holding one or more wire electrodes (4) each of which passes through an aperture (5) in a stent support bar (6), means for moving the stent support bar (6) towards or away from the electrode support member (3) in a direction along or each the electrode (4), the or each wire electrode (4) having a diameter which is less than the predetermined stent internal diameter (*d*) and a length such that they can extend beyond the stent support bar (6) by a distance which is greater than the predetermined stent length (*l*), and further comprising one or more contact positioning members (7) selectively movable in relation to the or each electrode (4) for urging contact between each such electrode (4) and a stent (2) carried thereby.
2. A jig (1) according to claim 1 wherein the electrode support member (3) holds a plurality of generally parallel wire electrodes (4).
3. A jig (1) according to claim 1 or claim 2, wherein said stent support bar (6) is movable between first and second positions and the or each contact positioning member (7) is located at a distance of between  $l/3$  and  $2l/3$  from the nearer of such positions, *l* being the predetermined stent length.
4. A jig (1) according to any preceding claim, wherein the or each contact positioning member (7) is annular and means is provided for moving the or each member (7) in an orbital manner about a wire electrode (4).

5. A stent processing plant incorporating one or more stent processing bath, at least one jig (1) according to any preceding claim, and means for transporting said jig and immersing it in successive processing baths. 5
6. A method of processing one or more stents (2) in at least one liquid bath, wherein the or each stent (2) to be processed is placed on a jig (1) comprising one or more wire electrodes (4) in such manner that the or each electrode (4) passes through and projects beyond the full length of a stent (2) placed thereon, wherein the or each stent (2) carried by the jig (1) is immersed in a liquid bath which contains an electrolyte and the or each stent (2) is urged into contact with its associated electrode (4) while current is applied to the electrode (4), and wherein positions of contact between the stent (2) and its respective electrode (4) is altered during processing without removing the stent (2) from the jig (1). 10 15 20
7. A method according to claim 6, wherein processing of the or each stent (2) is performed in a succession of liquid baths while the or each stent (2) is carried by the same jig (1). 25
8. A method of processing a stent (2) in a liquid bath comprising holding a wall of the stent (2) between an inner member (8) extending into the stent (2) and engaging an inner surface of the wall of the stent (2) and an outer member (7) engaging an outer surface of the wall of the stent (2); and changing the contact positions at which the inner (8) and outer (7) members contact the wall of the stent (2) so as to expose that part of the wall that was previously obscured by the members (8,7), the changing of the contact positions being performed without removing the stent (2) from the inner member (8). 30 35
9. A method according to claim 8 in which the diameter of the inner member (8) is substantially less than the internal diameter of the stent (2), and in which changing of the contact positions is effected by relative movement between the inner member (8) and the wall of the stent (2) so as to disengage the inner member (8) from a first portion of the inner wall of the stent (2) and engage it with a different second portion of the inner wall of the stent. 40 45
10. A method according to claim 8 or claim 9 in which it is a different inner member (8) that contacts the inner wall of the stent (2) at different times so as to expose previously obscured stent wall. 50
11. A method according to any of claims 8 to 10 in which it is a different outer member (7) that contacts the outer wall at different times. 55
12. A method according to any of claims 8 to 11 comprising extending the inner member (8) substantially completely through the elongate length of the stent (2), or beyond the elongate length of the stent (2).
13. A method according to any of claims 8 to 12 in which the inner member (8) or the outer member (7) comprises an electrode and the processing of the stent (2) comprises an electrolytic process.
14. A liquid bath treatment jig (1) adapted to treat stents (2), the jig (1) comprising:
  - a set of a plurality of first stent-engaging formations adapted to be inserted inside respective stents;
  - a complementary set of a plurality of second stent-engaging formations adapted to engage an outside wall of respective stents;
  - pairs of first and second formations being adapted to hold a stent (2) between them at a first position on the stent (2), when the formations are in a first position relative to each other;
  - pairs of the first and second formations being adapted to hold a stent (2) at a different, second, position on the stent (2) so as to expose said first position on the stent (2), in use, to liquid of the bath, when the formations are in a second position relative to each other;
  - and in which movement of the sets of first stent-engaging formations relative to the second set of stent-engaging formations is adapted to occur without removing the stents (2) from the first formations.
15. A method of producing a stent (2) using a pre-treatment or post-treatment bath and an electrolytic treatment bath comprising using a jig (1) to hold the stent (2), the jig (1) being the same jig (1) for pre-treatment/post-treatment and for electrolytic treatment, and the jig (1) having a stent-penetrating member that is introduced inside the stent (2), pressing the stent-penetrating member to the wall of the stent during the electrolytic treatment, and not positively urging the stent penetrating member against the inside of the stent (2) during pre-treatment or post-treatment, thereby facilitating the ingress of liquid between the stent penetrating member and the inner wall of the stent (2).
16. Stent processing apparatus comprising an electrolytic bath, a pre-or post- electrolytic treatment bath, a stent-carrying jig (1), and jig transport means adapted to move the jig (1) from bath to bath; the jig (1) having a stent-penetrating member adapted to be urged against the inside of the stent (2) when the jig (1) is placed in the electrolytic bath, and de-

biasing means adapted to ensure that the stent-penetrating means is not urged against the stent (2) when the jig (1) is in the pre- or post-treatment bath.

5

10

15

20

25

30

35


40

45


50

55

7

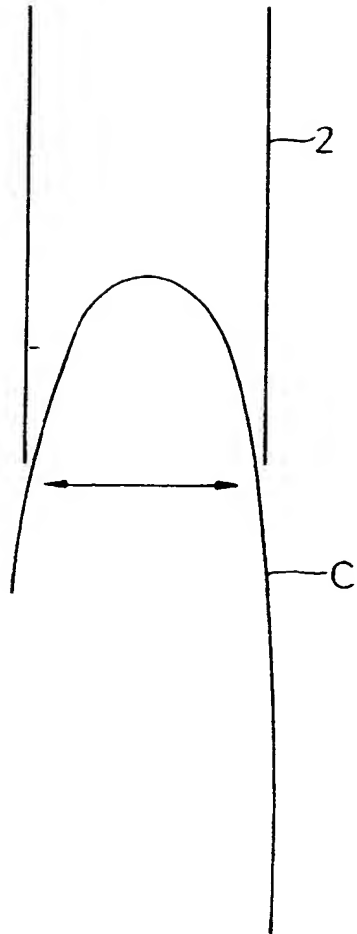


***Fig. 1A***  
(PRIOR ART)

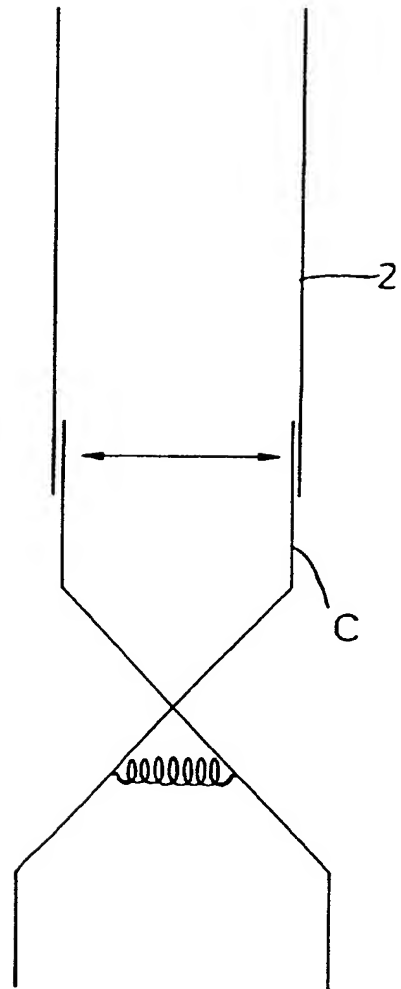


***Fig. 1B***  
(PRIOR ART)




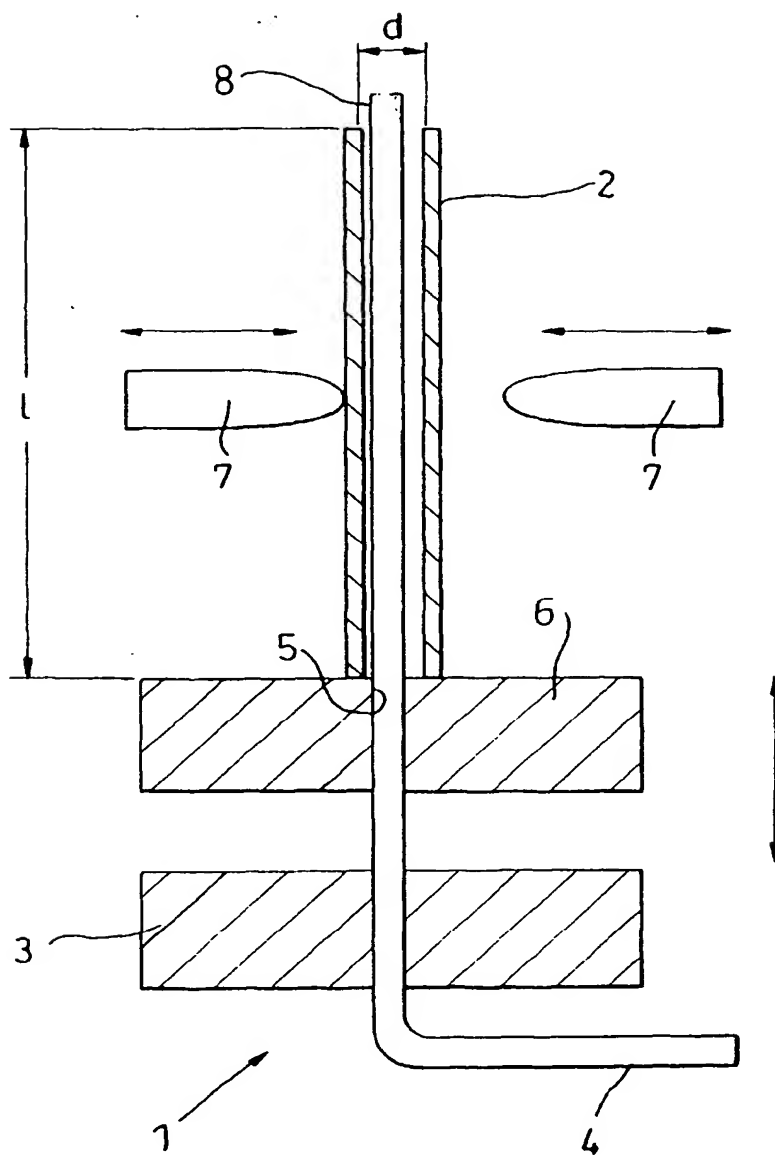


**Fig. 2**

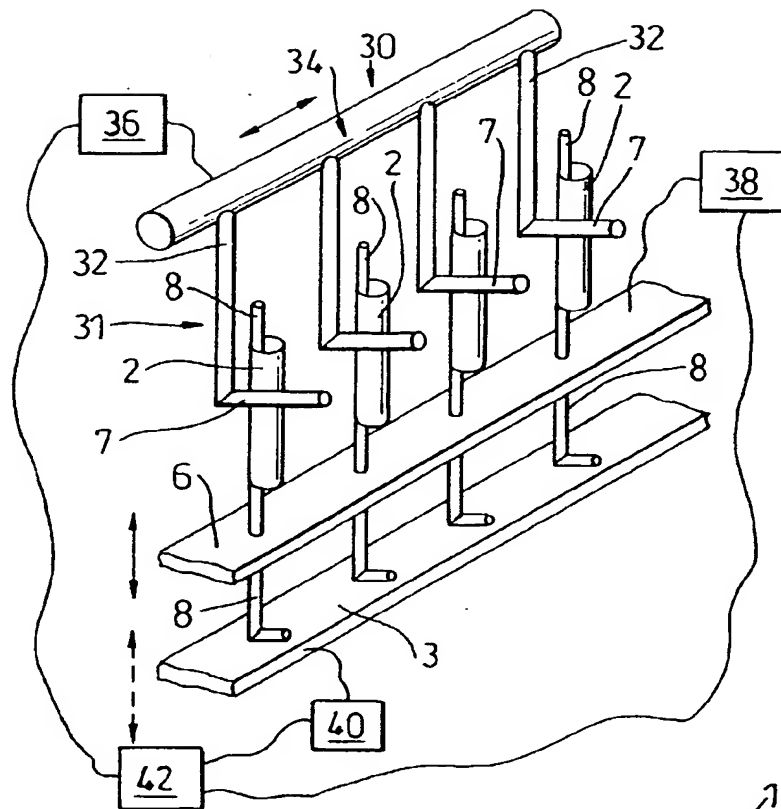


**Fig. 3**

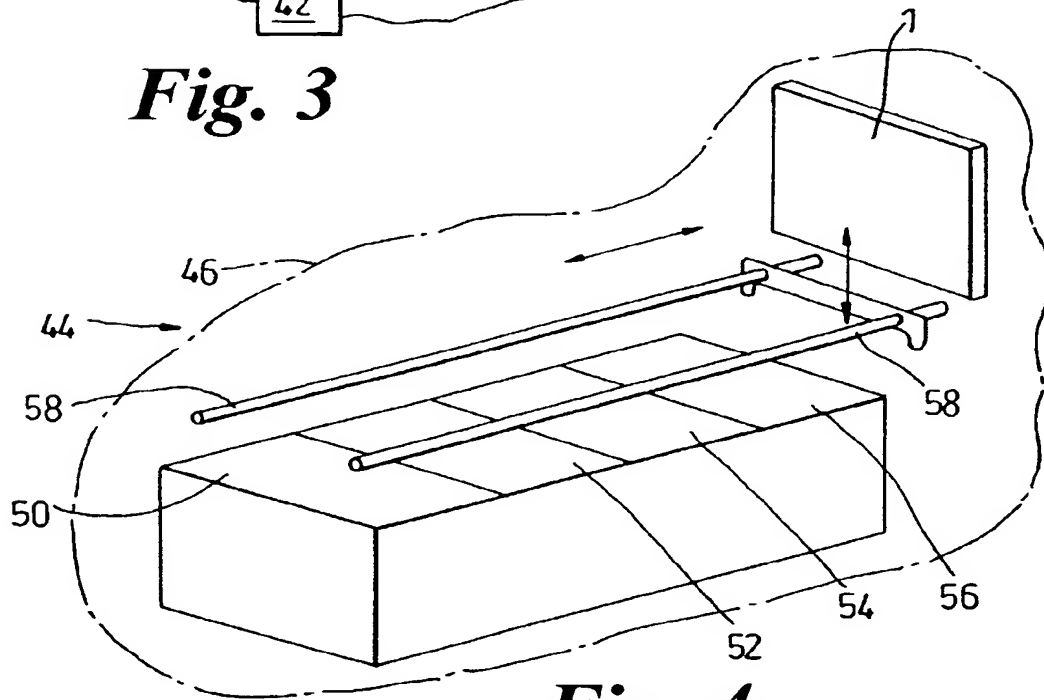


**Fig. 4**

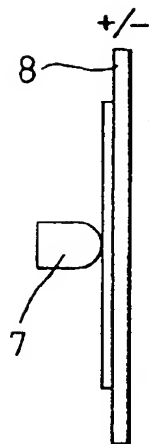


**Fig. 5A**

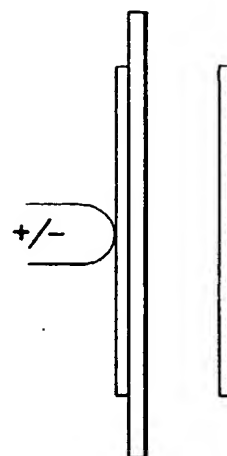


**Fig. 5B**

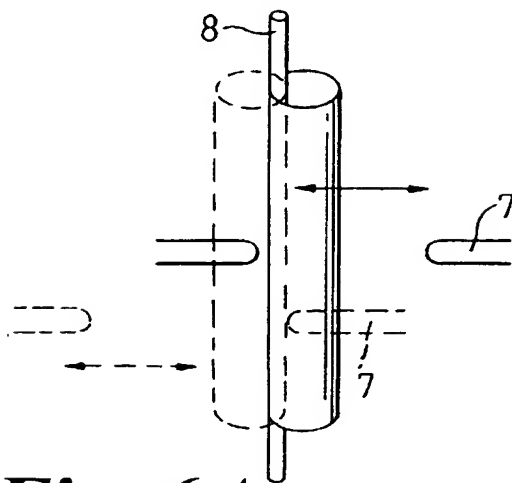


**Fig. 6A**

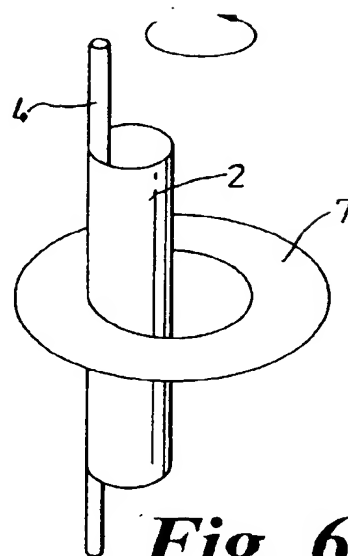


**Fig. 6B**

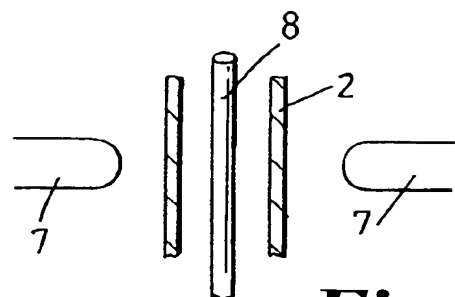


**Fig. 7**

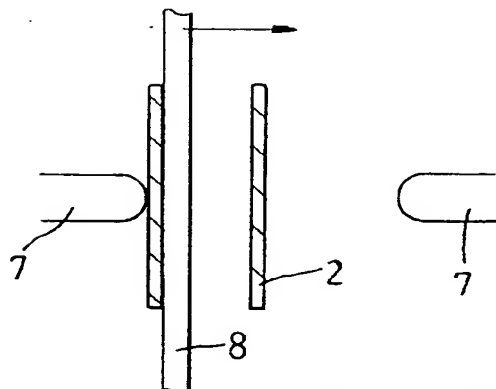

***Fig. 8A***

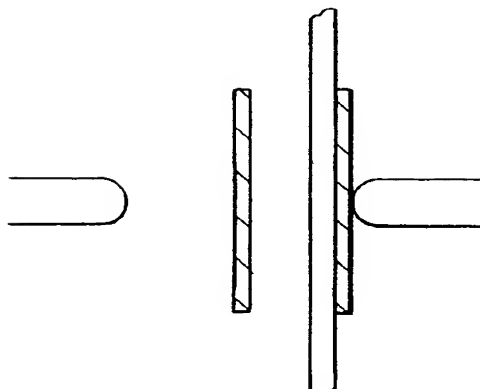

***Fig. 8B***

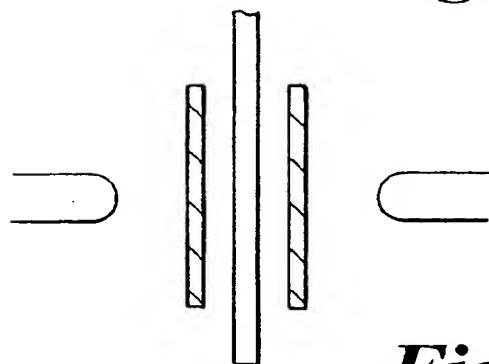

***Fig. 8C***

(19)



Europäisches Patentamt  
European Patent Office  
Office européen des brevets



(11)

**EP 1 369 099 A3**

(12)

**EUROPEAN PATENT APPLICATION**

(88) Date of publication A3:  
31.03.2004 Bulletin 2004/14

(51) Int Cl.7: **A61F 2/06, C25D 17/06**

(43) Date of publication A2:  
10.12.2003 Bulletin 2003/50

(21) Application number: **03253608.8**

(22) Date of filing: **06.06.2003**

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR  
HU IE IT LI LU MC NL PT RO SE SI SK TR**  
Designated Extension States:  
**AL LT LV MK**

(72) Inventor: **Swain, Brian**  
**Tamworth, Staffordshire B77 5AS (GB)**


(74) Representative: **Lawrence, John**  
**Barker Brettell**  
**138 Hagley Road**  
**Edgbaston**  
**Birmingham B16 9PW (GB)**

(30) Priority: **06.06.2002 GB 0212909**

(71) Applicant: **Anopol Limited**  
**Birmingham B5 5QJ (GB)**

**(54) Improvements in stent manufacture**

(57) Stents (2) to be processed in one or more liquid baths are placed on a jig (1) comprising a plurality of wire electrodes (4) in such manner that each electrode (4) passes through and projects beyond the full length of a stent (2) placed thereon. The stents (2) carried by the jig (1) are immersed in a liquid bath which contains an electrolyte and the stents (2) are urged into contact with their associated electrodes (4) while current is applied to those electrodes. The positions of contact between the stents (2) and their respective electrodes (4) are altered during processing without removing the stents from the jig (1). The method is applicable for electro polishing and electro-plating. The stents (2) may remain on the same jig (1) throughout processing. Also disclosed is a jig (1) suitable for performing the method and comprising an electrode support member (3) holding a plurality of generally parallel wire electrodes (4) each of which passes through a hole (5) in a stent support bar (6), means for moving the stent support bar (6) towards or away from the electrode support member (3) in a direction along the electrodes (4). The wire electrodes (4) each have a diameter less than the internal diameter of the stents (2) to be processed, and they extend beyond the stent support bar (6) by a distance which is greater than the length of the stents (2). A plurality of contact positioning members (7) are movable in relation to the electrodes (4) for urging contact between each such electrode (4) and a stent (2) carried thereby.

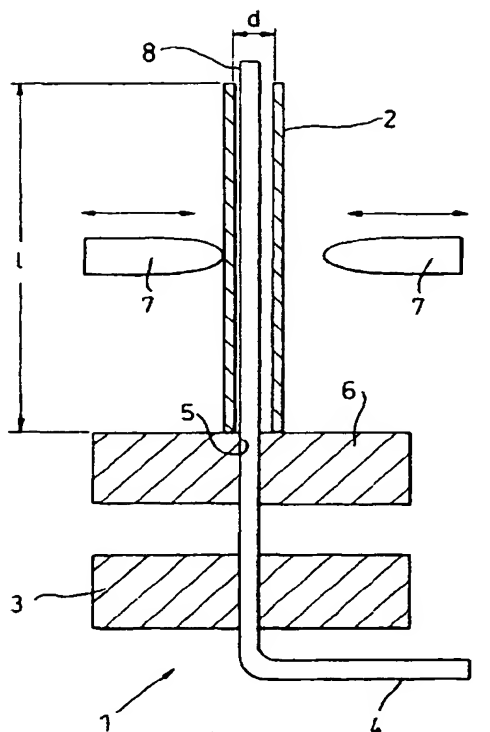

**Fig. 2**

**EP 1 369 099 A3**



European Patent  
Office

# EUROPEAN SEARCH REPORT

Application Number  
EP 03 25 3608

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.Cl.7)
A	WO 98/29025 A (MEDINOL LTD) 9 July 1998 (1998-07-09) * page 51, line 24 - page 54, line 20 * * figures 46-48 * * claims 59-66 *	1-5	A61F2/06 C25D17/06
A	FR 1 377 075 A (VMW RANSHOFEN BERNDORF AG) 31 October 1964 (1964-10-31) * page 1, column 2, paragraph 8 * * figures 1,2 *	1,2	
A	US 1 783 885 A (GRIMSHAW MARTIN FRANCIS ET AL) 2 December 1930 (1930-12-02) * page 3, line 120 - page 4, line 2 * * figure 3 *	1	
<p>-----</p> <p>The present search report has been drawn up for all claims</p>			<p>TECHNICAL FIELDS SEARCHED (Int.Cl.7)</p> <p>A61F C25D C25F</p>
Place of search		Date of completion of the search	Examiner
Munich		6 October 2003	Skorovs, P
<p>CATEGORY OF CITED DOCUMENTS</p> <p>X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document</p> <p>T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons &amp; : member of the same patent family, corresponding document</p>			

EPO FORM 1503 03.02 (P04C01)



European Patent  
Office

Application Number

EP 03 25 3608

### CLAIMS INCURRING FEES

The present European patent application comprised at the time of filing more than ten claims.

- ☐ Only part of the claims have been paid within the prescribed time limit. The present European search report has been drawn up for the first ten claims and for those claims for which claims fees have been paid, namely claim(s):
- ☐ No claims fees have been paid within the prescribed time limit. The present European search report has been drawn up for the first ten claims.

### LACK OF UNITY OF INVENTION

The Search Division considers that the present European patent application does not comply with the requirements of unity of invention and relates to several inventions or groups of inventions, namely:

see sheet 8

- ☐ All further search fees have been paid within the fixed time limit. The present European search report has been drawn up for all claims.
- ☐ As all searchable claims could be searched without effort justifying an additional fee, the Search Division did not invite payment of any additional fee.
- ☐ Only part of the further search fees have been paid within the fixed time limit. The present European search report has been drawn up for those parts of the European patent application which relate to the inventions in respect of which search fees have been paid, namely claims:
- ☒ None of the further search fees have been paid within the fixed time limit. The present European search report has been drawn up for those parts of the European patent application which relate to the invention first mentioned in the claims, namely claims:

1-5



European Patent  
Office

LACK OF UNITY OF INVENTION  
SHEET B

Application Number

EP 03 25 3608

The Search Division considers that the present European patent application does not comply with the requirements of unity of invention and relates to several inventions or groups of inventions, namely:

1. claims: 1-5

A jig for supporting stents in a liquid comprising a wire electrode; an electrode support member; a stent support bar; means for moving the stent support bar; and a contact positioning member for urging contact between the electrode and the stent.

---

2. claims: 6-7

A method for processing a stent in liquid baths, wherein the stent to be processed is placed on a jig comprising a wire electrode in such manner that the electrode passes through the full length of the stent, wherein the stent is urged into contact with electrode.

---

3. claims: 8-13

A method of processing a stent in a liquid bath, comprising: holding a wall of the stent between an inner member extending into the stent and engaging an inner surface of the wall of the stent; and an outer member engaging an outer surface of the wall of the stent.

---

4. claim: 14

A liquid bath treatment jig adapted to treat stents, comprising: a set of plurality of first stent-engaging formations adapted to be inserted inside respective stents; a complementary set of plurality of second stent-engaging formations adapted to engage an outside wall of respective stents.

---

5. claim: 15

A method of producing a stent using baths, comprising: a jig to hold a stent having stent-penetrating member that is introduced inside the stent and pressing the stent.

---

6. claim: 16

A stent processing apparatus, comprising: baths; and jig transport means adapted to move the jig from bath to bath; the jig having a stent-prenetrating member adapted to be urged against the inside of the stent.

---



**ANNEX TO THE EUROPEAN SEARCH REPORT  
ON EUROPEAN PATENT APPLICATION NO.**

EP 03 25 3608

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on  
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

06-10-2003

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 9829025	A	09-07-1998	US 5906759 A	25-05-1999
			AU 739820 B2	18-10-2001
			AU 4923997 A	02-07-1998
			AU 5876298 A	31-07-1998
			BR 9715033 A	28-02-2001
			CA 2225764 A1	26-06-1998
			CN 1185977 A	01-07-1998
			CZ 9704160 A3	15-07-1998
			DE 19757888 A1	02-07-1998
			EE 9700349 A	15-10-1998
			EE 200200308 A	15-10-2002
			EE 200200309 A	15-10-2002
			EE 200200310 A	15-10-2002
			EE 200200311 A	15-10-2002
			EP 0853927 A2	22-07-1998
			WO 9829025 A2	09-07-1998
			IL 122767 A	17-09-2003
			JP 10244008 A	14-09-1998
			NO 976076 A	29-06-1998
			NO 20025481 A	29-06-1998
			NZ 329481 A	25-08-2000
			NZ 501876 A	27-09-2002
			NZ 516882 A	29-08-2003
			PL 324018 A1	06-07-1998
			RU 2209094 C2	27-07-2003
			SG 87087 A1	19-03-2002
			SG 93226 A1	17-12-2002
			SK 177597 A3	14-02-2000
			US 5997703 A	07-12-1999
			US 6299755 B1	09-10-2001
			US 6197048 B1	06-03-2001
			US 6114049 A	05-09-2000
FR 1377075	A	31-10-1964	AT 235655 B	10-09-1964
			CH 413538 A	15-05-1966
			DE 1262725 B	07-03-1968
			GB 1057148 A	01-02-1967
US 1783885	A	02-12-1930	GB 299071 A	22-10-1928
			DE 472937 C	08-03-1929
			FR 641037 A	26-07-1928
			NL 22352 C	

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

**THIS PAGE BLANK (USPTO)**

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☒ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**

**THIS PAGE BLANK (USPTO)**